


MASS SPECTROMETRY REPORT

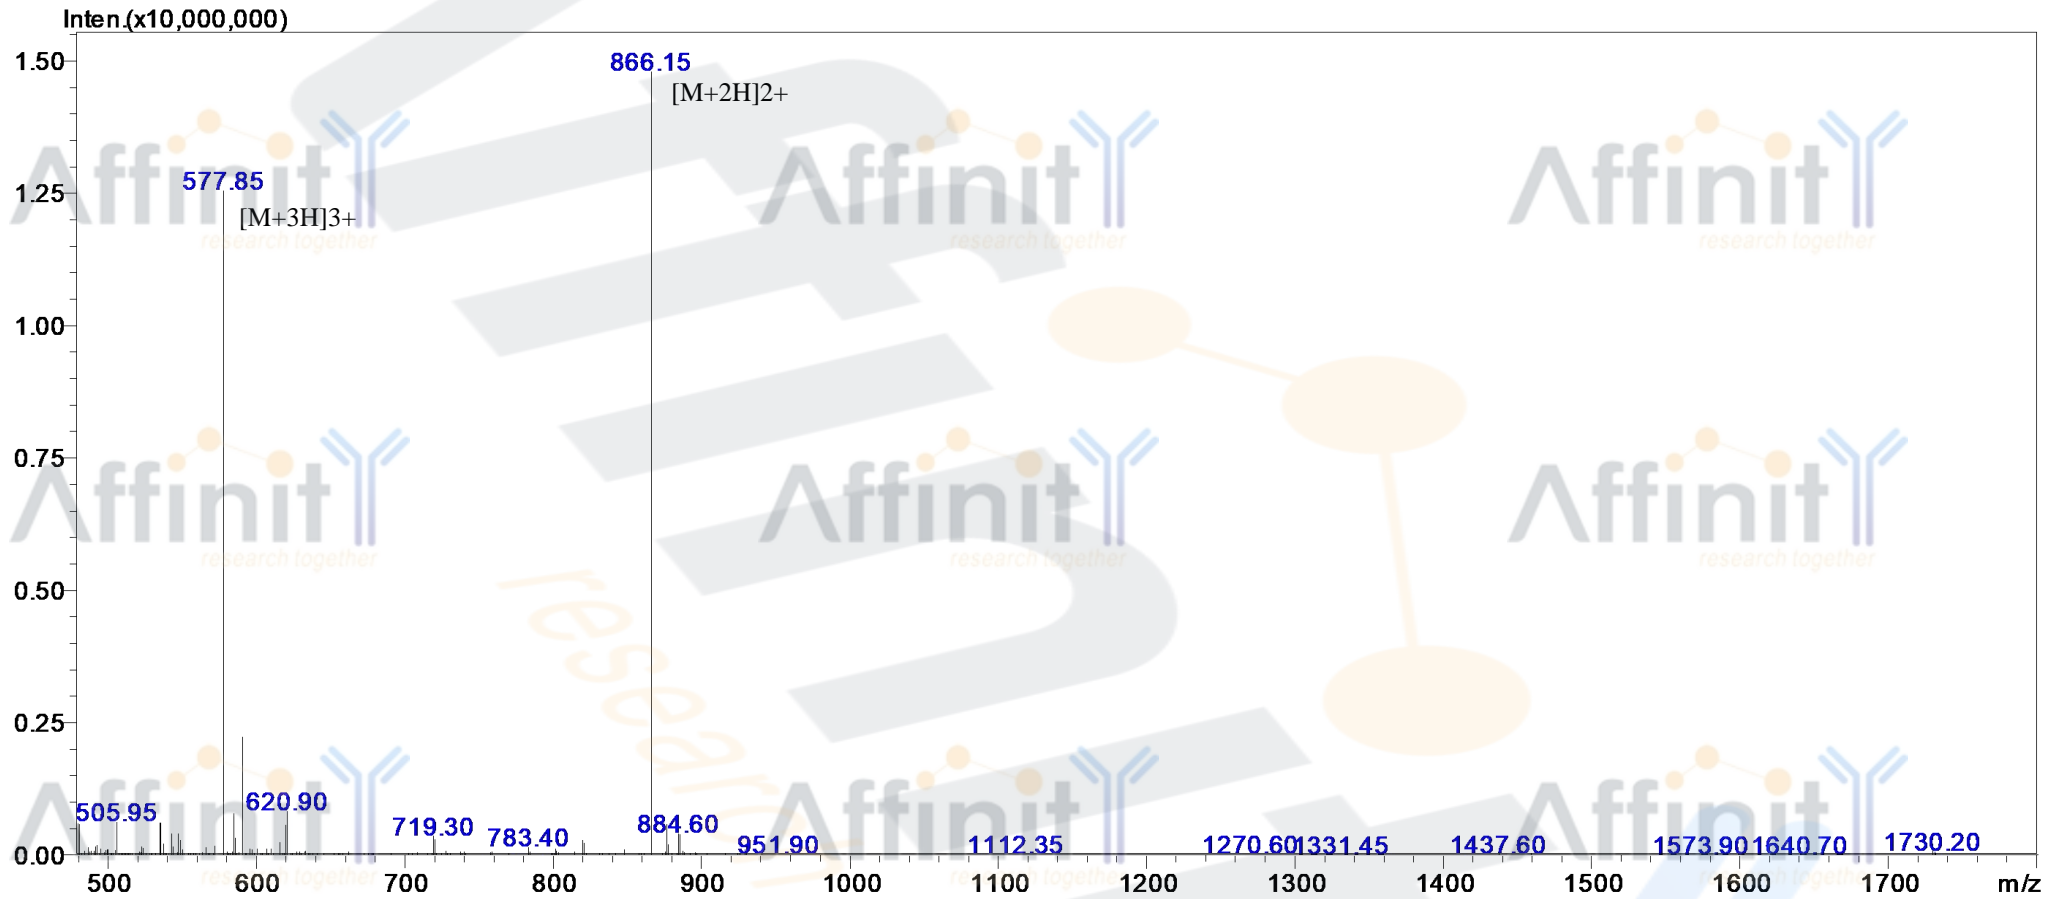

Sample Description

Analyzed date: 2013-7-17  
 Analyst: FENG  
 Sample: 5-307 CS-14  
 M.W.: 1730.03  
 Lot. No.: P130705-XZ358241

Instrument

SHIMADZU LCMS-2010EV  
 Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp.: 250 °C  
 Block Temp.: 200 °C  
 Probe Bias: + 4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. Conc.: 50% H<sub>2</sub>O/50% ACN